

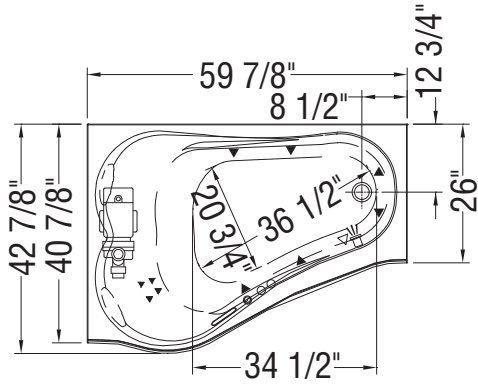


MICRO-JETS SYSTEM

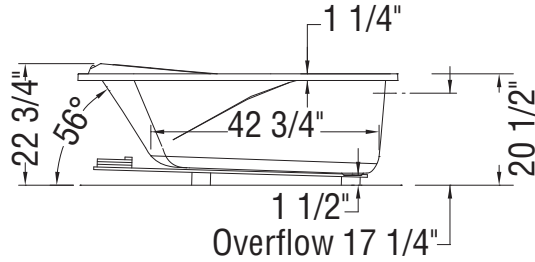

HYDROSENS, BACKMAX
AND AIR SYSTEM

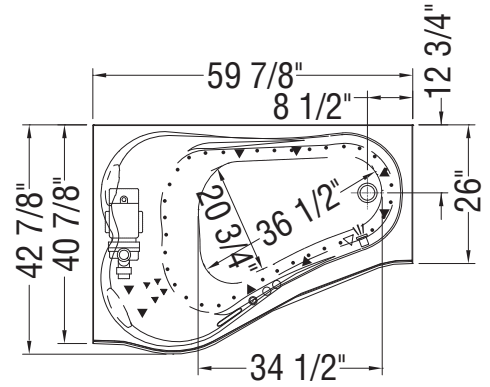

- (▲): Indicates whirlpool and backjets positioning
- (△): Indicates suction positioning
- (●): Indicates airjets positioning
- (☞): Indicates chromatherapy light positioning

All dimensions are approximate. Structure measurements must be verified against the unit to ensure proper fit.